Goode, et al.
Atty Docket: DEXCOM.025A Appl. No.: Unknown

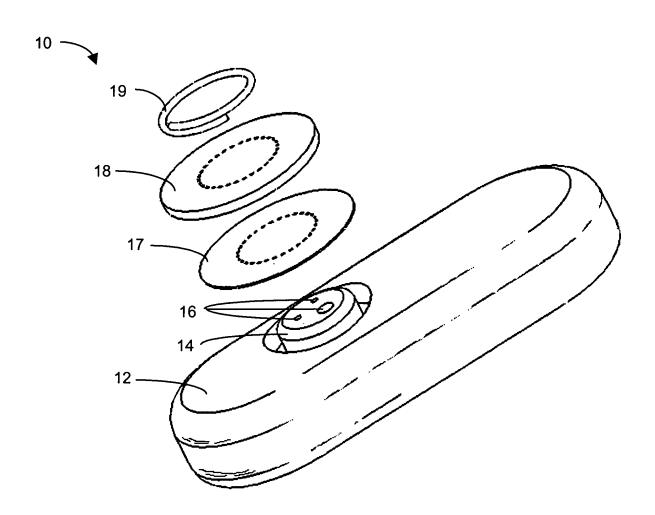


FIG. 1

SYSTEM AND METHODS FOR PROCESSING ANALYTE SENSOR DATA

Goode, et al.

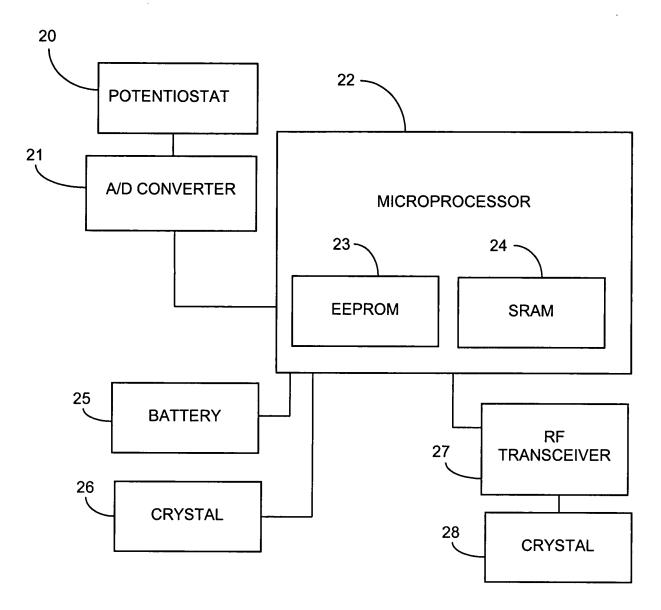


FIG. 2

SYSTEM AND METHODS FOR PROCESSING ANALYTE SENSOR

DATA
Goode, et al.
Atty Docket: DEXCOM.025A Appl. No.: Unknown

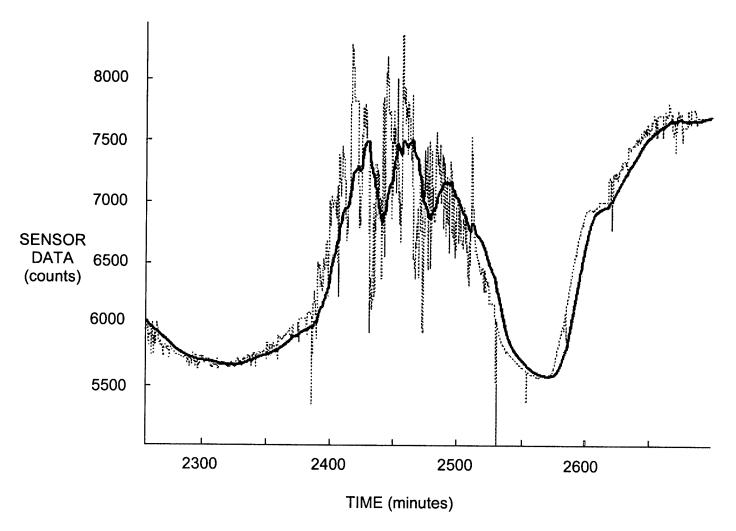


FIG. 3

Goode, et al.

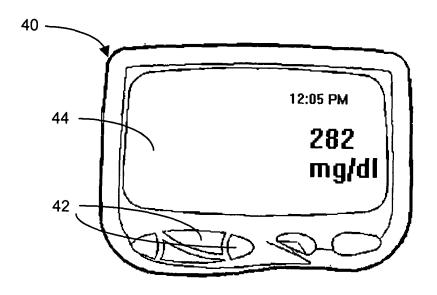


FIG. 4A

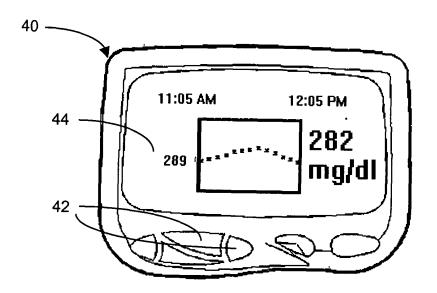


FIG. 4B

Goode, et al.

Appl. No.: Unknown

Atty Docket: DEXCOM.025A

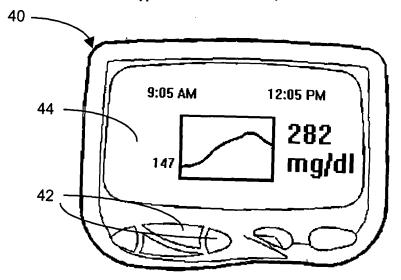


FIG. 4C

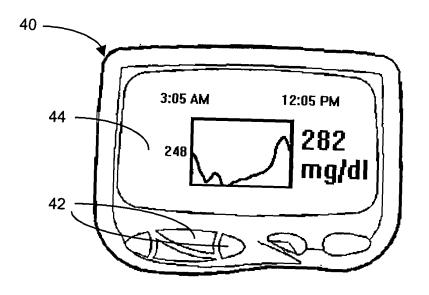


FIG. 4D


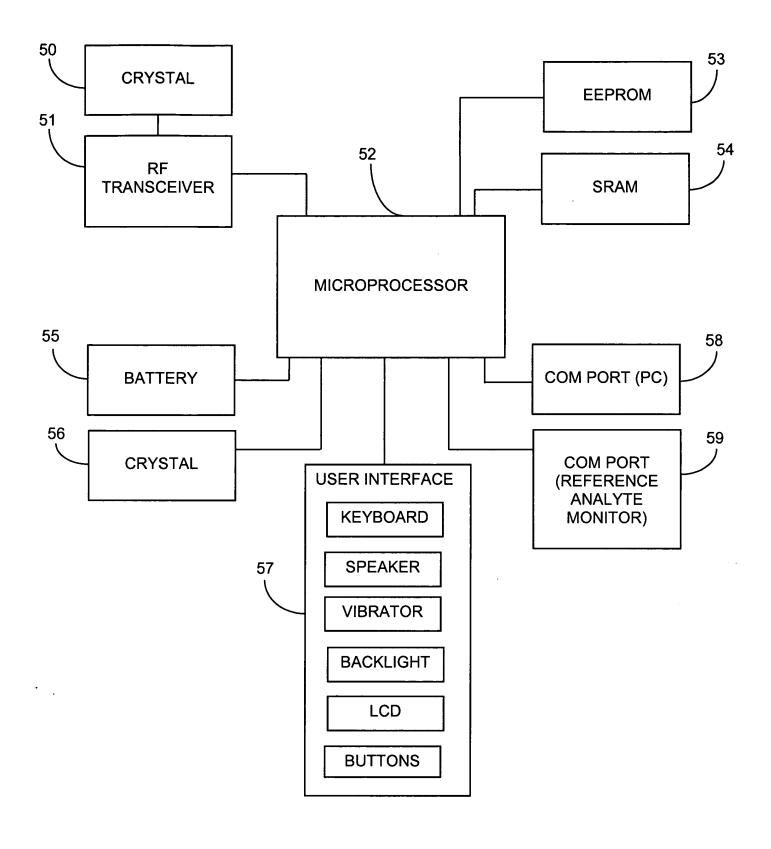


FIG. 5


Appl. No.: Unknown

Atty Docket: DEXCOM.025A

Goode, et al.

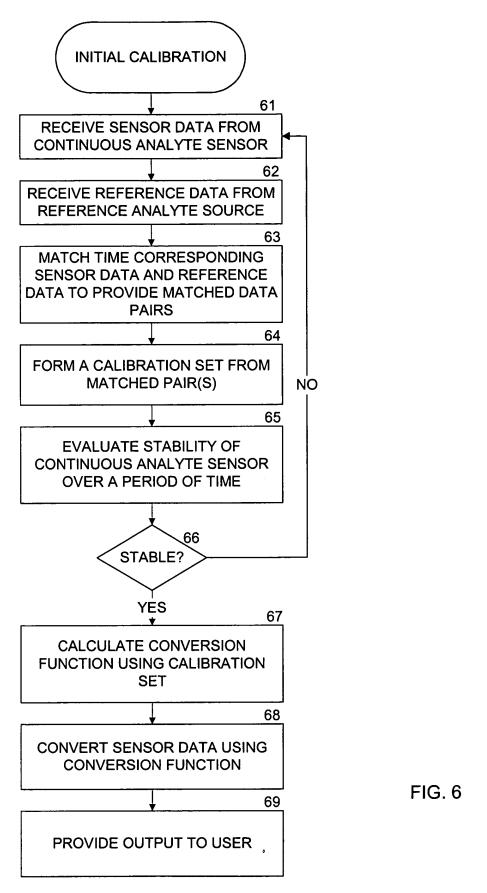

Appl. No.: Unknown

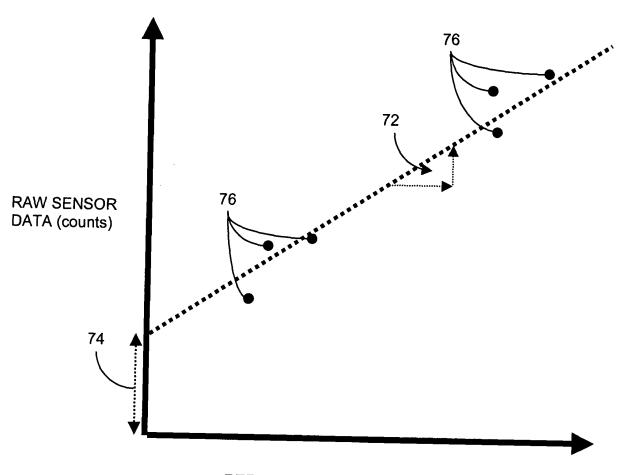

REFERENCE ANALYTE VALUE (mg/dL)


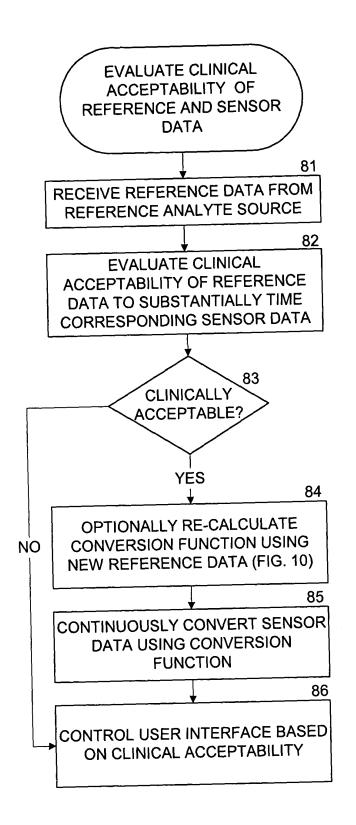


FIG. 8

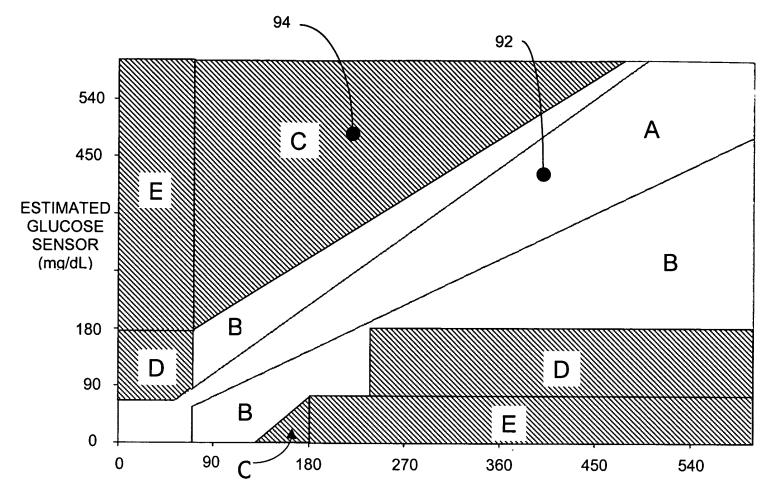

REFERENCE GLUCOSE VALUE (mg/dL)

FIG. 9

SYSTEM AND METHODS FOR PROCESSING ANALYTE SENSOR DATA

Goode, et al.

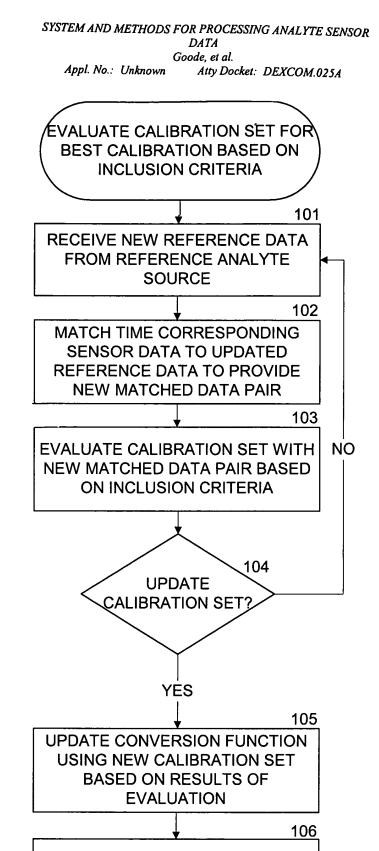


FIG. 10

CONVERT SENSOR DATA USING UPDATED CONVERSION FUNCTION

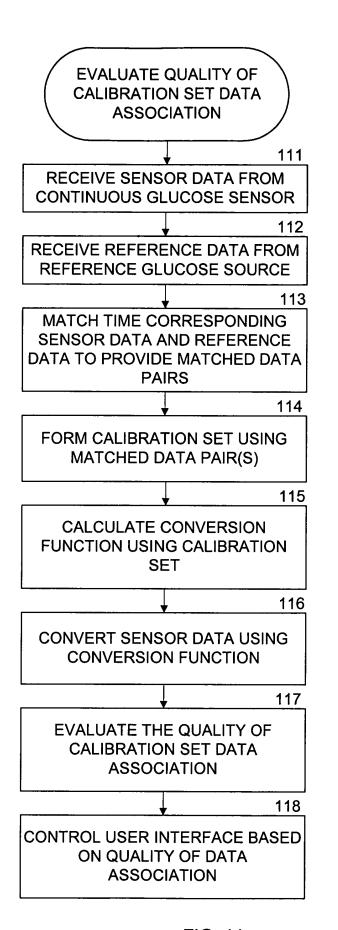
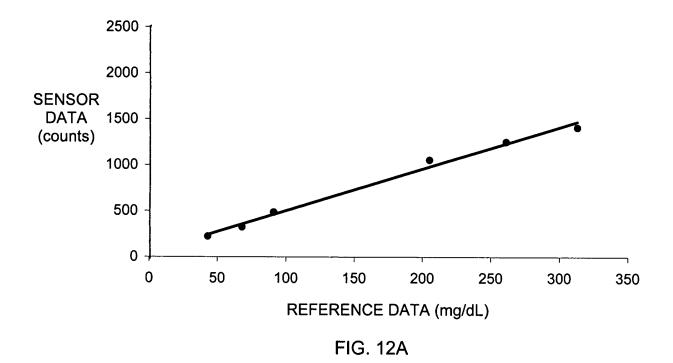


FIG. 11



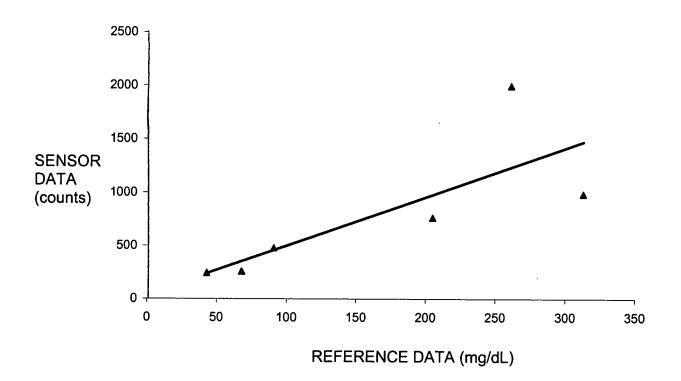


FIG. 12B